


Thermo Scientific Dionex AS-AP Sample Conductivity and pH Accessory

Automated Sample Measurement and Method Selection

The Thermo Scientific Dionex AS-AP Sample Conductivity and pH Accessory is designed to streamline IC workflows that require sample conductivity and pH measurements before injection. This customer-installable option for the Dionex AS-AP Autosampler offers a whole new level of convenience, time-savings, and increased productivity by allowing automatic calibration and measurement of sample conductivity and pH, subsequent sample handling using conditional statements, and reporting, all within the dimensions of the Dionex AS-AP Autosampler.

- In-line measurements of conductivity and pH before injecting samples onto the column
- Utilization of conditional statements in the Thermo Scientific Dionex Chromeleon Chromatography Data System to allow user to make automated sample injection decisions
- Automatic reporting – Readings are displayed in the sequence report column and post-run reports
- Seamless integration with the Dionex AS-AP Autosampler

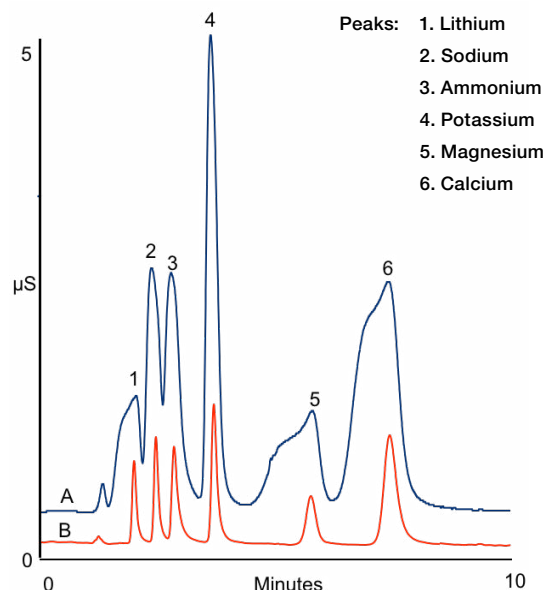

High-concentration cation standard, separated using a Thermo Scientific Dionex IonPac CS12A, 3 × 150 mm column.

A. Without AS-AP Sample Conductivity and pH Accessory.

Standard injection of 25 μ L is performed, leading to column overloading and poor chromatography.

B. With AS-AP Sample Conductivity and pH Accessory.

Because sample conductivity measures above a set threshold, the Chromeleon™ software automatically adjusts the injection volume to 2.5 μ L. Analytes are well resolved with the lower volume injection.



Thermo
SCIENTIFIC

Conductivity and pH readings can be displayed in report columns on the sequence table for easy review.

No	Name	pH	conductivity [µS]	Pos.	Inj. Vol	Status	Program	Method	Inj. Date/Time	Sample Temp [°C]
1	di water	5.52	0	RA1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 11:09:26	29.0
2	di water	5.23	0	RA1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 11:21:35	28.6
3	cal_pH7	n.a.	n.a.	RB1	0.40	Finished	cal_pH7_method 1	WaterMethod	1/6/2012 11:24:41	28.6
4	cal_pH4	n.a.	n.a.	RB2	0.40	Finished	cal_pH4_method 1	WaterMethod	1/6/2012 11:35:20	28.5
5	cal_pH10	n.a.	n.a.	RB3	0.40	Finished	cal_pH10_end_method 1	WaterMethod	1/6/2012 11:46:01	28.1
6	Sample_pH7	7.00	7414	RB1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 12:05:42	28.1
7	Sample_pH4	4.00	4355	RB2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 12:17:51	28.2
8	Sample_pH10	9.95	11867	RB3	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 12:30:00	28.3
9	Sample_200 uS	8.42	199	RB4	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 12:42:08	28.3
10	Sample_1000 uS	6.29	1003	RB5	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 12:54:17	28.3
11	Sample_2000 uS	6.08	2016	RC1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 1:06:25 P	28.4
12	Municipal Water	7.87	472	RC2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 1:18:33 P	28.4
13	Municipal Water	7.89	472	RC2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 1:30:42 P	28.4
14	Municipal Water	7.91	473	RC2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 1:42:50 P	28.5
15	Chiller sample	5.12	903	RC3	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 1:54:58 P	28.5
16	Chiller sample	5.06	904	RC3	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 2:07:07 P	28.5
17	Chiller sample	4.93	903	RC3	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 2:19:14 P	28.6
18	boiler sample	11.64	4523	RD1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 3:44:12 P	28.7
19	boiler sample	11.65	4519	RD1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 3:56:19 P	28.8
20	boiler sample	11.64	4511	RD1	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 4:08:27 P	28.7
21	water sample 1	8.65	637	RD2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 4:20:35 P	28.5
22	water sample 1	8.59	637	RD2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 4:32:43 P	28.5
23	water sample 1	8.57	638	RD2	0.40	Finished	measure pH_cond_method 1	WaterMethod	1/6/2012 4:44:51 P	28.5

DIONEX AS-AP SAMPLE CONDUCTIVITY AND PH ACCESSORY SPECIFICATIONS

Type	Conductivity: Flow-through; pH: Flow-through, silver/silver-chloride electrode
Conductivity Range	0.0 to 30,000 µS
Conductivity Accuracy	At 1000 µS, +/- 0.3%, at point of calibration
Conductivity Minimum Sample Volume	500 µL
pH Range	pH 2 to 12
pH Accuracy	Better than +/- 0.1 pH units at point of calibration (pH 4, 7, and 10), including sensor
pH Minimum Sample Volume	1500 µL (2000 µL recommended)
Control Software	Chromeleon software version 7.1 SR1 or higher Chromeleon software version 6.8 SR10 + DU10c or higher. Supports Microsoft Windows® 7, Vista, and XP

Ordering Information

P/N	Product	Content
074923*	AS-AP Sample Conductivity and pH Accessory	AS-AP Conductivity and pH module, pH probe, and mounting kit
075529*	AS-AP Sample Conductivity and pH Accessory pH Electrode	Ag/AgCl-pH Electrode
074123*	Valve Assembly, includes one 2-Way, 6-Port Valve and Mounting Hardware	6-Port Valve and Mounting Hardware
070209*	2-Way, 6-Port Valve†	6-Port Valve
588801-16**	1000 µS Conductivity Calibration Standard	500 mL bottle of 1000 µS Conductivity Standard
SB101-500**	pH 4 Calibration and Check Standard	500 mL bottle of pH 4 Standard Solution
SB107-500**	pH 7 Calibration and Check Standard	500 mL bottle of pH 7 Standard Solution
SB141-500**	pH 10 Calibration and Check Standard	500 mL bottle of pH 10 Standard Solution

† For Push mode, an AUX valve is required and for pH measurements, a 5 mL syringe and 8.5 mL buffer loop is recommended.

*Thermo Scientific part number.

**Fisher Scientific part number.

www.thermofisher.com

©2016 Thermo Fisher Scientific Inc. All rights reserved. Windows is a registered trademark of Microsoft Corporation. All other trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

U.S./Canada (847) 295 7500	Brazil (55) 11 3731 5140	India (91) 22 2764 2735	Singapore (65) 6289 1190
Australia (61) 2 9420 5233	China (852) 2428 3282	Ireland (353) 1 644 0064	Sweden (46) 8 473 3380
Austria (43) 1 616 51 25	Denmark (45) 36 36 90 90	Italy (39) 02 51 62 1267	Switzerland (41) 62 205 9966
Benelux (31) 20 683 9768	France (33) 1 39 30 01 10	Japan (81) 6 6885 1213	Taiwan (886) 2 8751 6655
(32) 3 353 42 94	Germany (49) 6126 991 0	Korea (82) 2 2653 2580	United Kingdom (44) 1276 691722

Thermo
SCIENTIFIC
Part of Thermo Fisher Scientific